


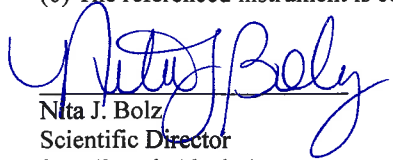
**VERIFICATION OF CALIBRATION REPORT***of DataMaster cdm Breath Test Instrument**State of Alaska**Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program*

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N <u>130116</u> ✓	
Name	<u>Steve Kevan</u>	ID#	<u>6585</u> ✓ Date <u>03/04/2011</u> ✓
A	Agency <u>Alaska State Troopers</u>	Phone #	<u>(907) 438-6500</u>
Instrument Location		<u>Emmonak AST Post</u>	
Alco S/N <u>77111</u> ✓		Target Value	<u>.078</u> ✓ High Pressure <u>700</u>
Alco Test Values		<u>.074</u> ✓	<u>.074</u> ✓
		1 <sup>st</sup> Alco	2 <sup>nd</sup> Alco
Signature			
(OVER)			


(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:


- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

  
 Nita J. Bolz  
 Scientific Director  
 State Breath Alcohol Program

Subscribed and sworn before me this 16 day of JUNE, 2010 2011

 (Notary Seal Stamp)  
 Carolyn M. Notland KYLE KLOPPER  
 Notary Public, State of Alaska  
 Commission Expires with Office

BT9 06/03



# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130116

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130116

MARCH 04, 2011

OPERATOR'S NAME: *BMB 6/14/11*  
KEVAN, STEVE  
OPERATOR'S NUMBER: 6585  
SUBJECT'S LAST NAME:  
TEST  
SUBJECT'S FIRST NAME/MI :  
TEST  
O.L. #: 00  
DEPT/AGENCY: ENH0  
CASE/REPORT: 00  
TEST TYPE: U  
ALCO TARGET VALUE: .078  
ALCO S/N: 77111

### --- BREATH ANALYSIS ---

.078 ADJUSTED FOR 30.50 in  
ALCO TARGET .079 13:24  
BLANK TEST .000 13:25  
INTERNAL STANDARD VERIFIED 13:25  
ALCO TV 30.50 in .074 13:26  
BLANK TEST .000 13:27  
SUBJECT SAMPLE *BMB 6/14/11* .000 13:27  
BLANK TEST .000 13:28  
ALCO TV 30.50 in .074 13:28  
BLANK TEST .000 13:29

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130116

MARCH 04, 2011  
TIME 13:22

### --- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 02/20/01  
HEATERS  
SAMPLE CHAMBER: 48c  
BREATH TUBE: 42c  
BAROMETER: 30.50 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

### PRINTER TEST

!"#\$%&'()\*+,-./0123456789:;<=>?@ABCDEF  
HIJKLMNOPQRSTUVWXYZ[\]^\_`abcdefgijklmno  
pqrstuvwxyz{|}~■